

Research Use Only. Not for use in diagnostic procedures.

## Anti-acetyl-Histone H3 Lysine 9 (H3K9ac) Acceptor Beads

**Product No.:** AL114C (250 µg)  
AL114M (5 mg)  
AL114R (25 mg)

**Lot No.:** 2906049

### Product Formats

Catalog #	Size	Volume	Assay points*
AL114C	250 µg	0.05 mL	500
AL114M	5 mg	1 mL	10 000
AL114R	25 mg	5 mL	50 000

\*The number of assay points is based on an assay volume of 25 µL using a final bead concentration of 20 µg/mL in 384-well format.

**Manufacturing Date:** August 6, 2021

### Product Information

**Description:** Anti-acetyl-Histone H3 Lysine 9 (H3K9ac) Acceptor beads at 5 mg/mL in PBS pH 7.2, supplemented with 0.05% Kathon as a preservative. Source of the antibody: rabbit monoclonal.

**Application:** This product is designed to detect human Histone H3 acetylated at lysine 9 (H3K9ac) in a homogeneous AlphaLISA® assay. Broad species cross-reactivity is expected based on sequence similarity.

**Storage:** Store in the dark at 4°C.

**Stability:** This product is stable for at least 12 months from the manufacturing date when stored in its original packaging at the recommended storage conditions.


**FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.**

### Quality Control

Lot-to-lot consistency is confirmed by a Quality Control AlphaLISA titration assay read on an EnVision® HTS Alpha instrument. Maximum signal and EC<sub>50</sub> value are determined using the biotin-H3K9ac peptide. Minimum signal is derived from the non-modified biotin-H3 peptide at the concentration giving the specified maximum signal. We certify that this product meets our quality release criteria. Maximum counts may vary between lots and depending on assay conditions.

Maximum signal: 1152338 counts  
Minimum signal: 27204 counts  
EC<sub>50</sub>: 0.93 nM

## Typical Data

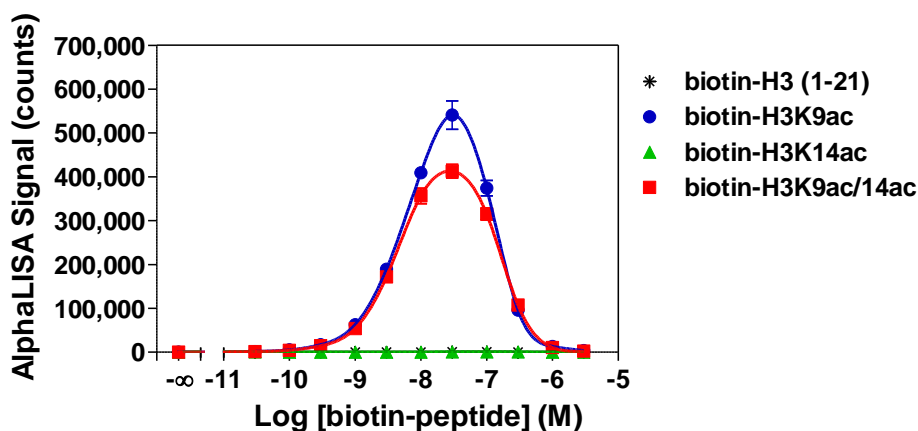

**Specificity of Anti-acetyl-Histone H3 Lysine 9 (H3K9ac) Acceptor Beads.** Histone H3-derived peptides with different epigenetic marks were titrated. Signal was detected with an EnVision® HTS Alpha instrument 2102. The hook effect observed at higher peptide concentrations is typical of three-component assays and occurs when peptide concentrations exceed the binding capacity of the Alpha Donor and/or AlphaLISA Acceptor beads.

A Technical Note presenting the optimization of an AlphaLISA p300 histone H3 lysine acetyltransferase assay using anti-H3K9ac Acceptor beads is available on our website at [www.perkinelmer.com/epigenetics](http://www.perkinelmer.com/epigenetics).

## Peptide Titration Assay

Peptide titration provides a means to verify product performance. It is used as our Quality Control release test. The following reagents and materials are recommended:

Item	Supplier	Catalog #
AlphaScreen® Streptavidin Donor Beads	PerkinElmer	6760002S (1 mg) 6760002 (5 mg) 6760002B (50 mg)
Histone H3 (K9ac) peptide, biotinylated	AnaSpec	64361
Histone H3 (1-21) peptide, biotinylated	AnaSpec	61702
AlphaLISA® 5X Epigenetics Buffer 1 Kit*	PerkinElmer	AL008C (10 mL Kit) AL008F (100 mL Kit)
White opaque OptiPlate™-384	PerkinElmer	6007290
TopSeal™-A Adhesive Sealing Film	PerkinElmer	6050195
EnSpire® or EnVision® Multilabel Alpha Reader	PerkinElmer	-

\*The two-component AlphaLISA 5X Epigenetics Buffer 1 Kit includes AlphaLISA 5X Epigenetics Buffer 1 and AlphaLISA 30X Buffer Supplement. The 1X AlphaLISA Epigenetics Buffer 1 may appear cloudy. However, this will not affect assay performance. The 1X Epigenetics Buffer 1 should be used within 16 hours.

These microplates can also be used with this product:

Item	Recommended Assay Volume	Supplier	Catalog #
White opaque OptiPlate-96	100 µL	PerkinElmer	6005290
White ½ AreaPlate-96	50 µL	PerkinElmer	6005560
Light gray AlphaPlate™-384	25 µL	PerkinElmer	6005350
ProxiPlate™-384 Plus	12.5 µL	PerkinElmer	6008280
Light gray AlphaPlate-1536	5 - 10 µL	PerkinElmer	6004350

## Recommendations

- AlphaScreen Donor beads are light-sensitive. All Alpha assays using the Donor beads should be performed under subdued laboratory lighting (< 100 lux). Green filters (LEE 090 filters (preferred) or Roscolux filters #389 from Rosco) can be applied to light fixtures.
- Sodium azide should not be added to the stock reagents. High concentrations of sodium azide (> 0.001 % final in the assay) might decrease the AlphaLISA signal.
- Spin down tubes briefly before use to improve recovery of content (2,000 x g, 10-15 sec). Resuspend all reagents by vortexing before use.
- Use Milli-Q® grade H<sub>2</sub>O (18 MΩ•cm) to prepare the 1X AlphaLISA Epigenetics Buffer 1.
- When diluting peptides, change tips after each dilution. When loading reagents in the assay microplate, change tips after each reagent addition and between each set of reagents.
- Small volumes may be prone to evaporation. It is recommended to cover microplates with a TopSeal-A Adhesive Sealing Film to reduce evaporation during incubation. Microplates are read with the TopSeal-A Film on the plate.
- Total signal varies with temperature and incubation time. For consistent results, identical incubation times and temperature should be used for all plates
- The AlphaLISA signal is detected with an EnSpire or EnVision Multilabel Reader equipped with the ALPHA option using the AlphaScreen standard settings (i.e. Total Measurement Time: 550 ms, Excitation Time: 180 ms, Mirror: D640as, Emission Filter: M570w, Center Wavelength 570 nm, Bandwidth 100 nm, Transmittance 75%).

## Quality Control Protocol

### PLEASE READ RECOMMENDATIONS ON PAGE 3 BEFORE USE


This titration protocol is designed for 12 dilutions of 2 peptides with triplicate determinations. Peptide concentrations are indicated for a 10  $\mu\text{L}$  volume. Final concentration of Alpha Donor and AlphaLISA Acceptor beads in the 25  $\mu\text{L}$  final assay volume is 20  $\mu\text{g}/\text{mL}$ . Volume of diluted reagents should be adjusted according to total assay points, plate format or assay volume.

- 1) Assay Buffer:  
The Assay Buffer used for biotin-peptide dilution is 50 mM Tris-HCl pH 8.0.
- 2) Serial dilutions of biotin-peptide in Assay Buffer:  
Prepare dilution series for each biotin-peptide as follows, changing tip for each dilution:

Tube	Volume of biotin-peptide	Volume of Assay Buffer ( $\mu\text{L}$ )	[biotin-peptide] (M) in 10 $\mu\text{L}$
A	12 $\mu\text{L}$ of 50 $\mu\text{M}$ stock	188	$3.0 \times 10^{-6}$
B	60 $\mu\text{L}$ of tube A	120	$1.0 \times 10^{-6}$
C	60 $\mu\text{L}$ of tube B	140	$3.0 \times 10^{-7}$
D	60 $\mu\text{L}$ of tube C	120	$1.0 \times 10^{-7}$
E	60 $\mu\text{L}$ of tube D	140	$3.0 \times 10^{-8}$
F	60 $\mu\text{L}$ of tube E	120	$1.0 \times 10^{-8}$
G	60 $\mu\text{L}$ of tube F	140	$3.0 \times 10^{-9}$
H	60 $\mu\text{L}$ of tube G	120	$1.0 \times 10^{-9}$
I	60 $\mu\text{L}$ of tube H	140	$3.0 \times 10^{-10}$
J	60 $\mu\text{L}$ of tube I	120	$1.0 \times 10^{-10}$
K	60 $\mu\text{L}$ of tube J	140	$3.0 \times 10^{-11}$
L	0	100	0

- 3) Preparation of 1X AlphaLISA Epigenetics Buffer 1:  
Add 2.0 mL of AlphaLISA 5X Epigenetics Buffer 1 and 0.33 mL of AlphaLISA 30X Buffer Supplement to 7.67 mL  $\text{H}_2\text{O}$ . The cloudy appearance of the buffer is normal. Use the 1X Epigenetics Buffer within 16 hours.
- 4) Preparation of 5X AlphaLISA Acceptor beads (100  $\mu\text{g}/\text{mL}$ ):  
Add 10  $\mu\text{L}$  of 5 mg/mL AlphaLISA Acceptor beads to 490  $\mu\text{L}$  of 1X AlphaLISA Epigenetics Buffer 1.
- 5) Preparation of 2.5X Streptavidin Donor Beads (50  $\mu\text{g}/\text{mL}$ ):  
Keep the beads under subdued laboratory lighting.  
Add 10  $\mu\text{L}$  of 5 mg/mL Streptavidin Donor beads to 990  $\mu\text{L}$  of 1X AlphaLISA Epigenetics Buffer 1.

6) In a white opaque OptiPlate-384 microplate:

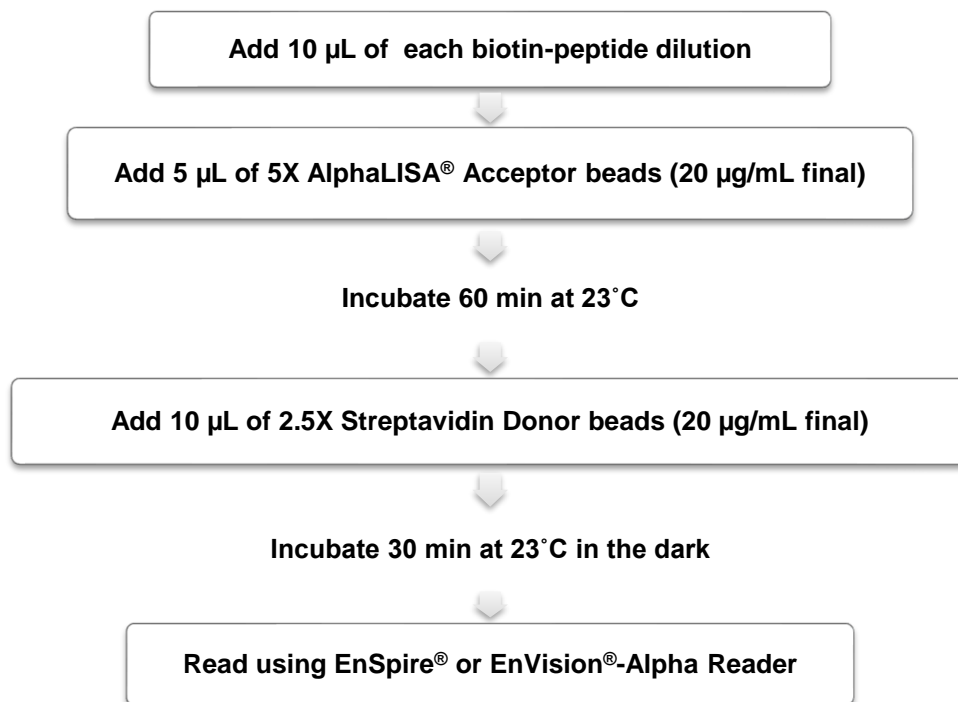

Please visit our website for additional information on the AlphaLISA technology at [www.perkinelmer.com/AlphaTech](http://www.perkinelmer.com/AlphaTech).

**This product is not for resale or distribution except by authorized distributors.**

**LIMITED WARRANTY:** PerkinElmer BioSignal Inc. warrants that, at the time of shipment, the products sold by it are free from defects in material and workmanship and conform to specifications which accompany the product. PerkinElmer BioSignal Inc. makes no other warranty, express or implied with respect to the products, including any warranty of merchantability or fitness for any particular purpose. Notification of any breach of warranty must be made within 60 days of receipt unless otherwise provided in writing by PerkinElmer BioSignal Inc. No claim shall be honored if the customer fails to notify PerkinElmer BioSignal Inc. within the period specified. The sole and exclusive remedy of the customer for any liability of PerkinElmer BioSignal Inc. of any kind including liability based upon warranty (express or implied whether contained herein or elsewhere), strict liability contract or otherwise is limited to the replacement of the goods or the refunds of the invoice price of goods. PerkinElmer BioSignal Inc. shall not in any case be liable for special, incidental or consequential damages of any kind.

PerkinElmer, Inc.  
940 Winter Street  
Waltham, MA 02451 USA  
P: (800) 762-4000 or  
(+1) 203-925-4602  
[www.perkinelmer.com](http://www.perkinelmer.com)



For a complete listing of our global offices, visit [www.perkinelmer.com/ContactUs](http://www.perkinelmer.com/ContactUs)

Copyright ©2010, PerkinElmer, Inc. All rights reserved. PerkinElmer® is a registered trademark of PerkinElmer, Inc. All other trademarks are the property of their respective owners.